
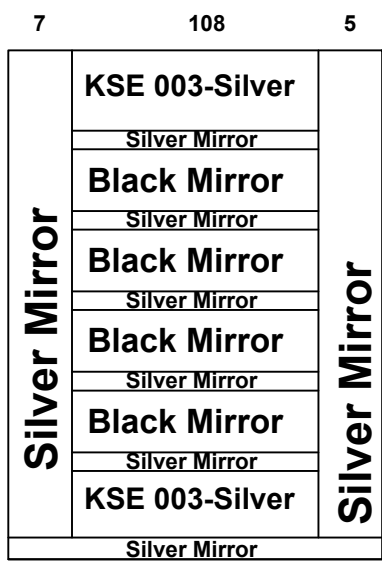
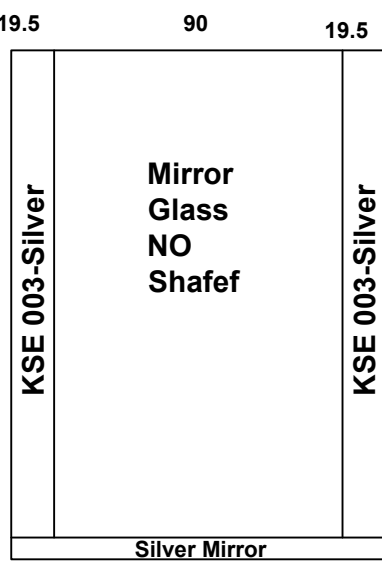


Date		Contract No.
29/11/2025		
Company		Customer
Meta ميتا		Crystal Medical Center مجمع الكرسنال الطبي
Pit	Over Hight	Motor Type
		Gearless 630
Guide Rails		

- Notes**
- 1- Flat Shoes 9mm
 - 2- All Pulley 18cm
 - 3-
 - 4-
 - 5-

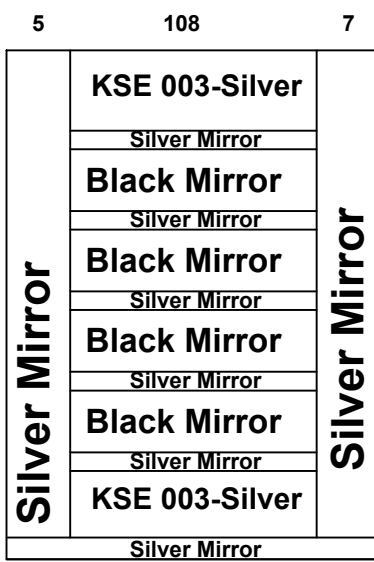

Options				Stainless Steel				Steel				 <p>Mirror Silver</p>
Handrail	2	LED			1.5 mm	3 mm	2 mm	G 1 mm				
Photocell	NO	NO			Marbel							
Wood					Request		Done					
5 mm		Colour	PVC	Type	ابيض صناعي معرق خفيف							
12 mm				Size	132.5x 119.5							
18 mm												